

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpakas vom Josefsberg/Eva Klingbacher
Josefsberg 11
9470 St. Paul Austria

Date: 06/26/18

Test No: 962495


Animal and Sample Description

Animal Name: AVJ Sir Marble
Breed: Alpaca(Huacaya)
Sex: Male
Color: Rose Grey

Animal ID: 276090010806073
Sample Location: Mid Side
Sample Date: 04/21/18
Age: 08/11/17

Laboratory Data

Mean Fiber Diameter:	15.9 microns	Fibers Greater Than 30 microns:	0.4 %
Standard Deviation:	3.5 microns	Comfort Factor:	99.6 %
Coefficient of Variation:	22.0 %	Mean Curvature:	44.9 deg/mm
Spin Fineness:	15.6 microns	SD Curvature:	26.9 deg/mm

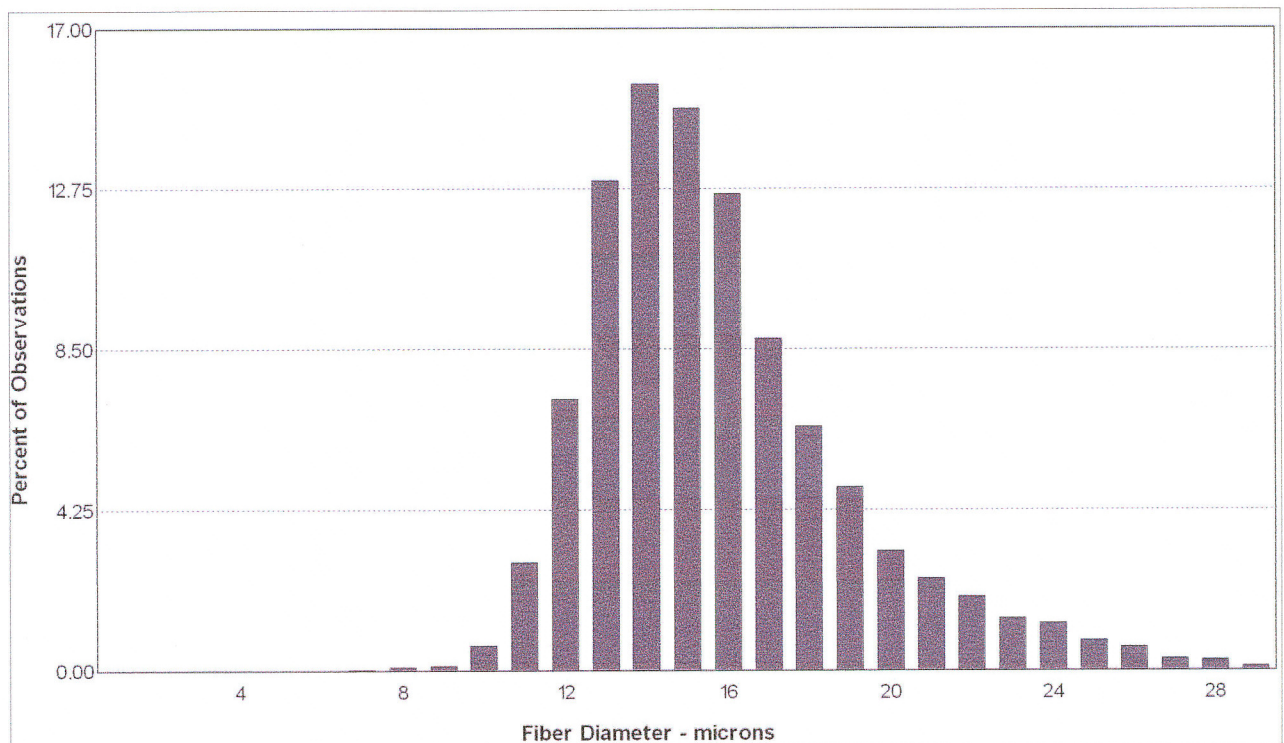

This Test Performed According to I.W.T.O Method 47