

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Westfalen Alpacas GbR/Tobias Topp & Patrick Budde  
Burbach 5  
48317 Drensteinfurt Germany

07/18/18

Test No: 963310


### Animal and Sample Description

**Animal Name:** WEST Voodoo ET  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Solid White

**Animal ID:** 967000010008338  
**Sample Location:** Side  
**Sample Date:** 04/02/18  
**Age:** 03/17/17

### Laboratory Data

<b>Mean Fiber Diameter:</b>	14.9 microns	<b>Spin Fineness:</b>	15.2 microns
<b>Standard Deviation:</b>	3.9 microns	<b>Mean Curvature (deg/mm):</b>	73.4
<b>Coefficient of Variation:</b>	26.1 %	<b>SD Curvature (deg/mm):</b>	40.9
<b>Fibers Greater Than 30 microns:</b>	0.6 %	<b>Comfort Factor:</b>	99.4 %
<b>Medullated Fibers:</b>	2.0 %		

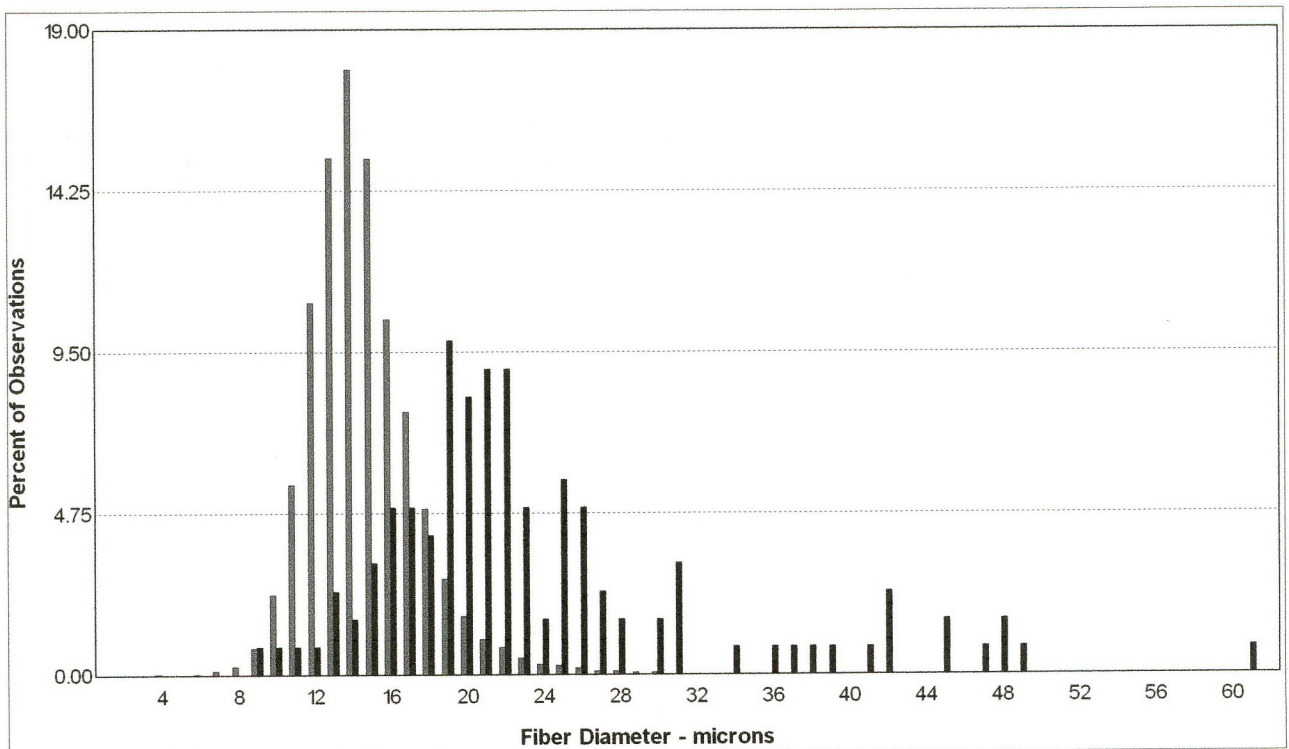

This Test Performed According to I.W.T.O Method 47